

topshelforthopedics.com
Phone: 866.592.0488 • Fax: 209.834.8832
Tracy, CA 95304
1851 East Paradise Road, Suite A
Topshelf
Manufacturing, LLC

BOA Compression Back Brace

Instructions for Use

Please read these instructions completely and carefully before applying this product. Correct application is important for proper function of this product.



BOA Compression Back Brace

Instructions for Use

Please read these instructions completely and carefully before applying this product. Correct application is important for proper function of the brace.

Indications: Acute and chronic low back pain, post-operative support, activity-related low back pain, and disc herniation.

Contraindications: Pregnancy and circulation, pulmonary, cardiovascular or skeletal conditions which have risk to be made worse as a result of compression and/or pressure.

1. Position and fasten the pull-handle as close as possible to the compression panels and fully extend the cord (Fig. 1).
2. Secure the anterior panel to the the brace by attaching the hook strip on the panel to the corresponding loop strip on the inside of the brace. Panel should extend approximately 5" beyond end of brace for proper fitting (Fig. 2 & 2A).
3. Referencing the attached label for correct brace orientation, position the brace around the waist and fasten. The pull-handle will be on the left side. The soft lining will be against the body (Fig. 3 & 3A).
4. For proper fit and compression, center the spine between the two side panels and position symmetrically on waist (Fig. 4).
5. To apply compression, grasp the pull-handle and pull to the right. After the desired level of compression is achieved, fasten the pull-handle to the contact strip on the side panels (Fig. 5 & 5A). A properly applied brace (Fig. 5B).

Chairback Application

- C1. Position and fasten the pull-handle as close as possible to the compression panels and fully extend the cord. Open the straps on the sides of the rigid frame. Place the brace around the rigid frame and center it. Fasten the straps on the rigid frame to secure the brace (Fig. C1). Apply the brace/frame combination around the waist. A properly applied brace (Fig. CA).

Using Lordotic Foam Inserts

- L1. Slide the appropriate insert (7, 10 or 12 degree) into the elastic pockets located on the inside of the side panels. Adjust for proper comfort (Fig. L1 & LA).

Use and Care:

The liner and straps may be hand washed with a mild detergent. Air dry only. Foam and straps may be trimmed and adjusted for proper fit.

Warning:










If you experience pain, swelling or sensation changes as a result of wearing this brace, consult your healthcare provider immediately. All adjustments of the brace should be done under the direction of a healthcare professional.

Warranty:



Top Shelf Orthopedics will replace all or part of the brace for defects in material or workmanship for the period of six months from the date of purchase.

Caution:

Federal Law (USA) restricts this device for sale by or on the order of a licensed healthcare professional.

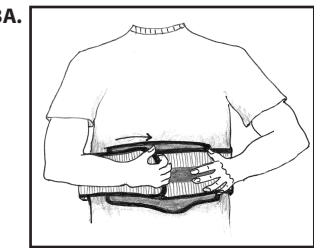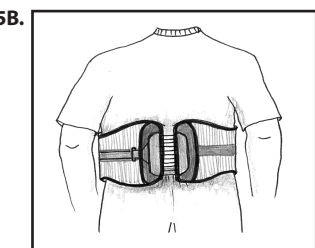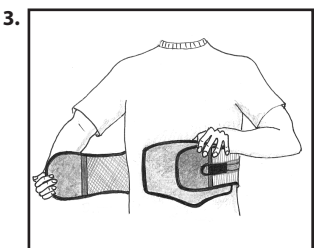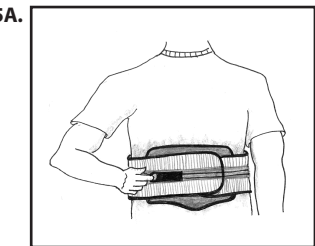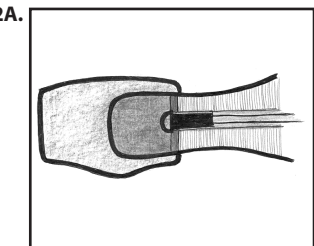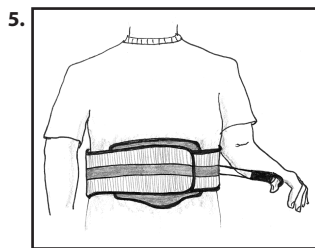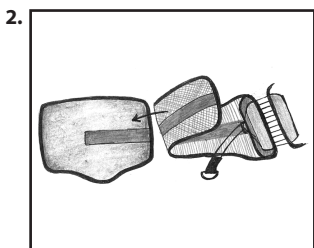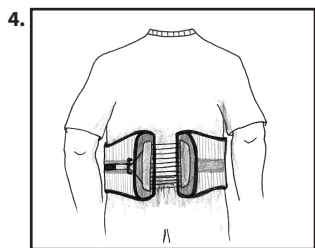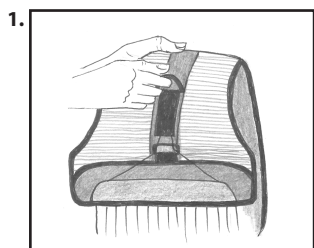

Chairback Application

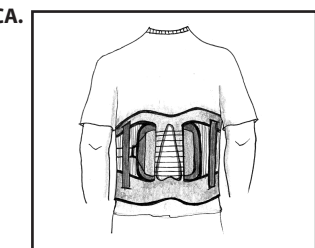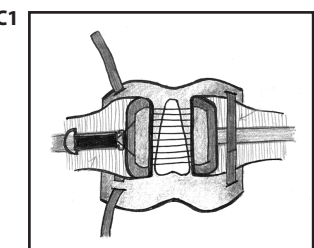

Lordotic Insert Application

